



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Wechselland Alpaka/Margot Wachabauer
Tauchen am Wechsel 61
7421 Tauchen am Wechsel Austria

Date: 02/18/19

Test No: 972704


Animal and Sample Description

Animal Name: AOG ZL Black Princess
Breed: Alpaca(Huacaya)
Sex: Female
Color: Black

Animal ID: 900200000021101
Sample Location: Side
Sample Date: 02/03/19
Age: 07/05/12

Laboratory Data

Mean Fiber Diameter:	23.4 microns	Fibers Greater Than 30 microns:	8.5 %
Standard Deviation:	5.2 microns	Comfort Factor:	91.5 %
Coefficient of Variation:	22.4 %	Mean Curvature:	30.4 deg/mm
Spin Fineness:	23.0 microns	SD Curvature:	18.9 deg/mm

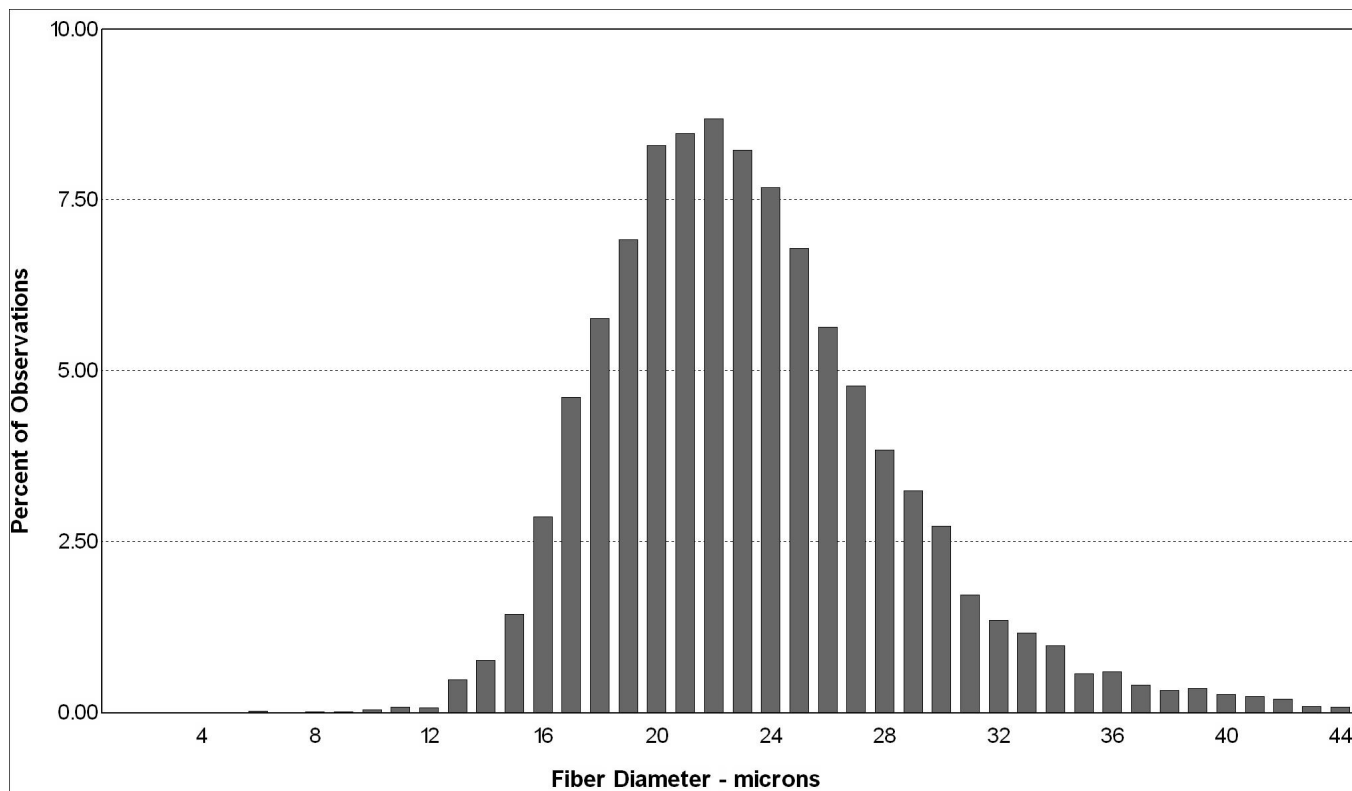

This Test Performed According to I.W.T.O Method 47