



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

WLA Wechselland Alpka/Fritz Wagner  
Tauchen 61  
Mönichkirchen 7421 Austria

03/13/20

Test No: 987884


### Animal and Sample Description

**Animal Name:** AOG ZL Black Princess  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** True Black

**Animal ID:** 90020000021101  
**Sample Location:** Side  
**Sample Date:** 03/01/20  
**Age:** 07/05/12

### Laboratory Data

<b>Mean Fiber Diameter:</b>	23.5 microns	<b>Spin Fineness:</b>	22.7 microns
<b>Standard Deviation:</b>	4.7 microns	<b>Medullated Fibers:</b>	0.0 %
<b>Coefficient of Variation:</b>	20.2 %	<b>Mean Curvature (deg/mm):</b>	32.6
<b>Fibers Greater Than 30 microns:</b>	7.5 %	<b>SD Curvature (deg/mm):</b>	22.5

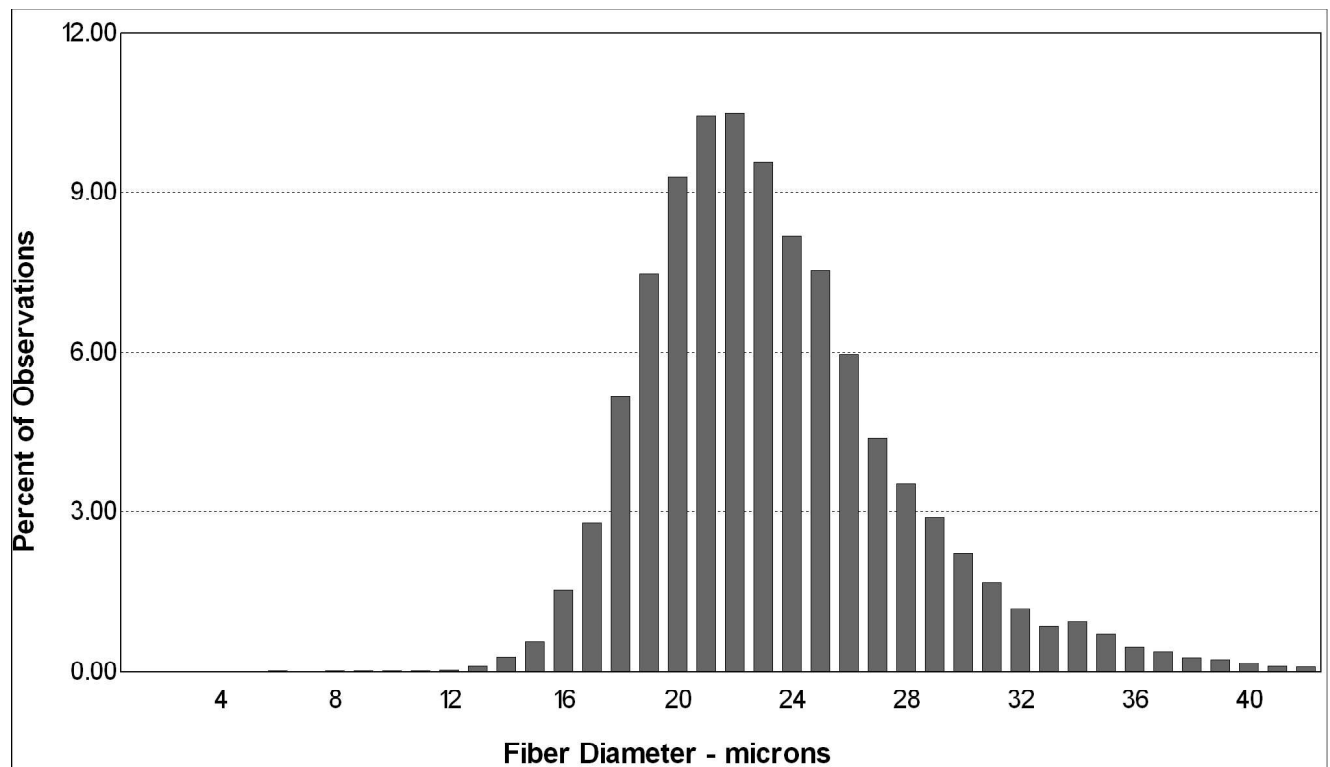

This Test Performed According to I.W.T.O Method 47