



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Wechselland Alpaka/Fritz Wagner
Tauchen 61
7421 Tauchen am Wechsel NÖ Austria

08/08/17

Test No: 947071


Animal and Sample Description

Animal Name: MMR Venola
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 941000001913479
Sample Location: Side (R)
Sample Date: 04/28/17
Age: 06/17/07

Laboratory Data

| | | | |
|--|--------------|---------------------------------|--------------|
| Mean Fiber Diameter: | 19.7 microns | Spin Fineness: | 19.3 microns |
| Standard Deviation: | 4.3 microns | Mean Curvature (deg/mm): | 57.3 |
| Coefficient of Variation: | 22.0 % | SD Curvature (deg/mm): | 40.9 |
| Fibers Greater Than 30 microns: | 2.5 % | Comfort Factor: | 97.5 % |

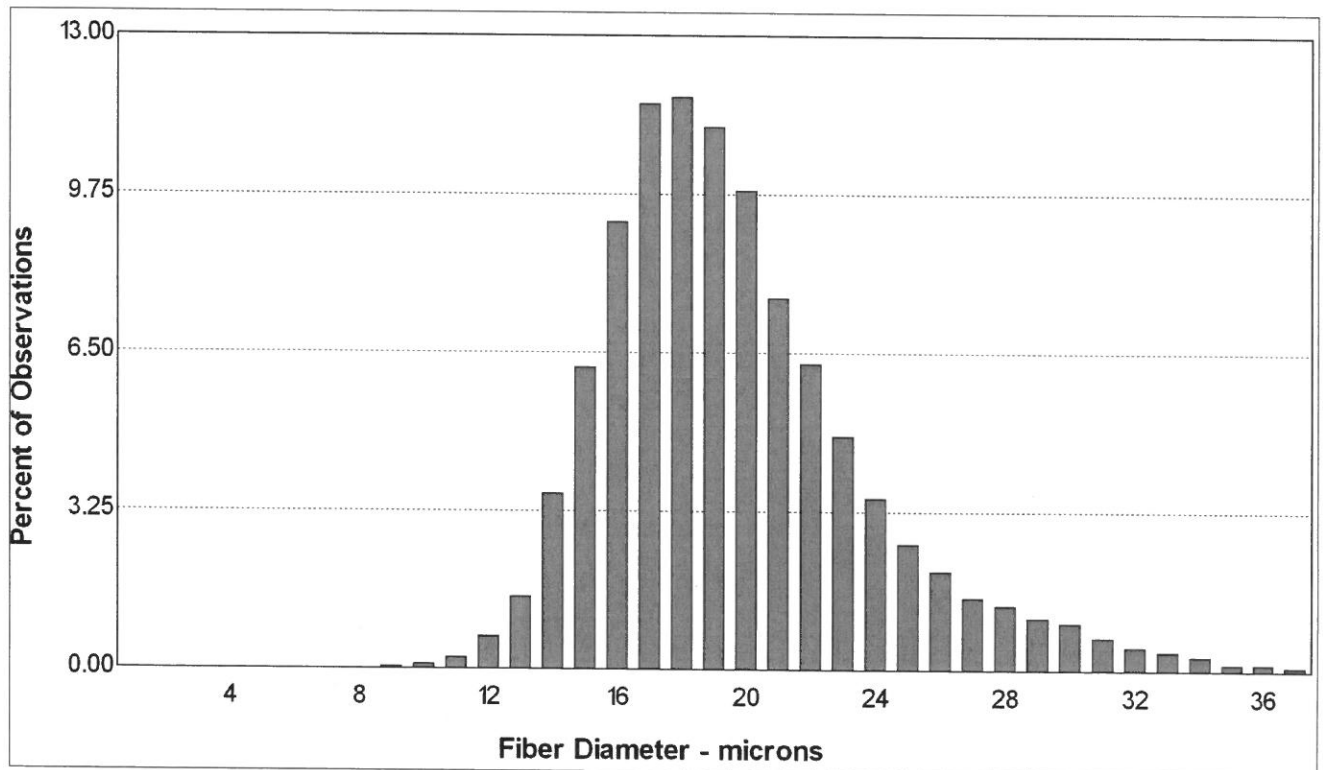

This Test Performed According to I.W.T.O Method 47