



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Wechselland Alpaka/Margot Wachabauer  
Tauchen am Wechsel 61  
7421 Tauchen am Wechsel Austria

**Date:** 02/18/19

**Test No:** 972703


### Animal and Sample Description

**Animal Name:** WLA Bailey  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Lt Fawn

**Animal ID:** 276093400739488  
**Sample Location:** Side  
**Sample Date:** 02/03/19  
**Age:** 07/24/18

### Laboratory Data

<b>Mean Fiber Diameter:</b>	17.2 microns	<b>Fibers Greater Than 30 microns:</b>	0.8 %
<b>Standard Deviation:</b>	3.8 microns	<b>Comfort Factor:</b>	99.2 %
<b>Coefficient of Variation:</b>	22.3 %	<b>Mean Curvature:</b>	41.7 deg/mm
<b>Spin Fineness:</b>	16.9 microns	<b>SD Curvature:</b>	24.0 deg/mm

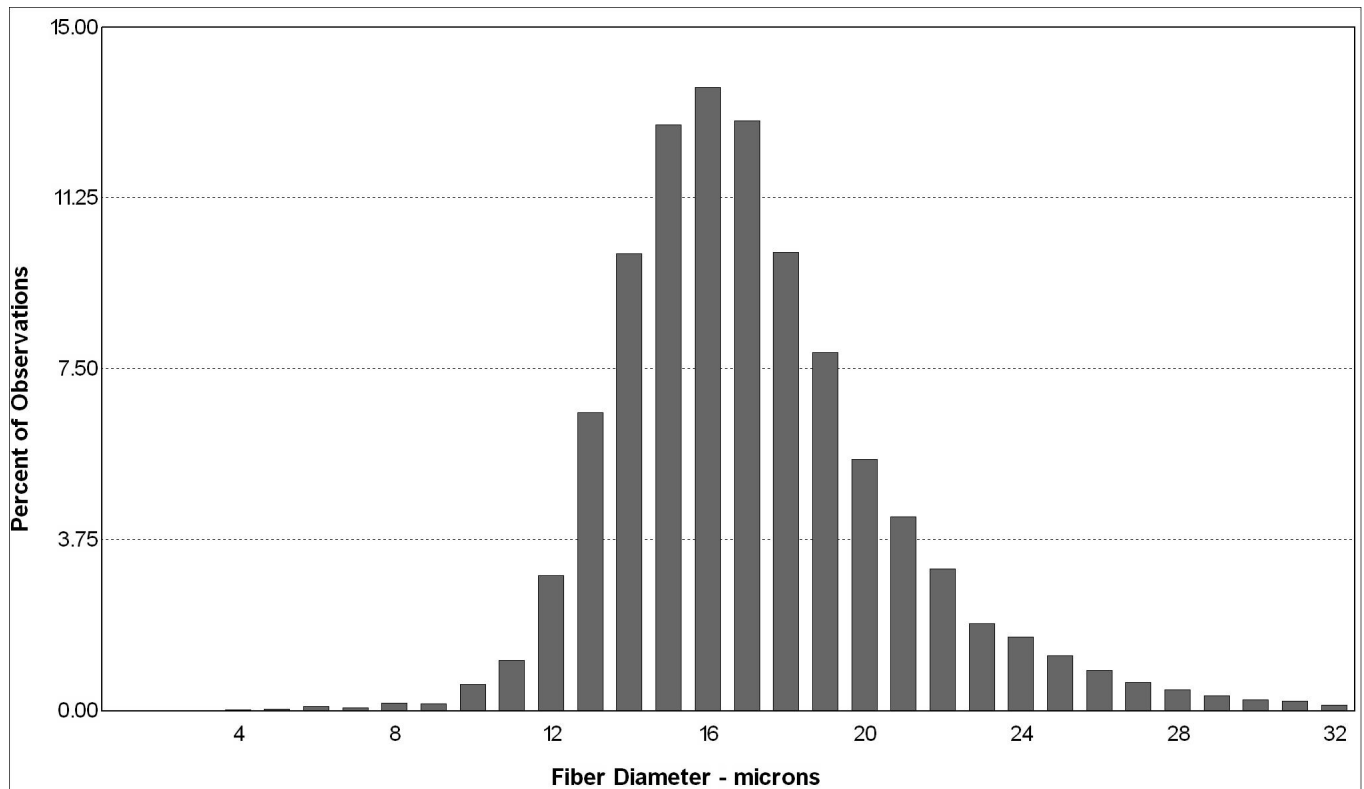

This Test Performed According to I.W.T.O Method 47