



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report**

Wechselland Alpaka/Fritz Wagner
Tauchen 61
7421 Tauchen am Wechsel NÖ Austria

06/13/18

Test No: 961510


Animal and Sample Description

Animal Name: WLA May Flower
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 276093480007425
Sample Location: Side (R)
Sample Date: 04/22/18
Age: 05/19/17

Laboratory Data

Mean Fiber Diameter:	19.1 microns	Spin Fineness:	18.3 microns
Standard Deviation:	3.7 microns	Mean Curvature (deg/mm):	42.2
Coefficient of Variation:	19.3 %	SD Curvature (deg/mm):	25.8
Fibers Greater Than 30 microns:	1.0 %	Comfort Factor:	99.0 %

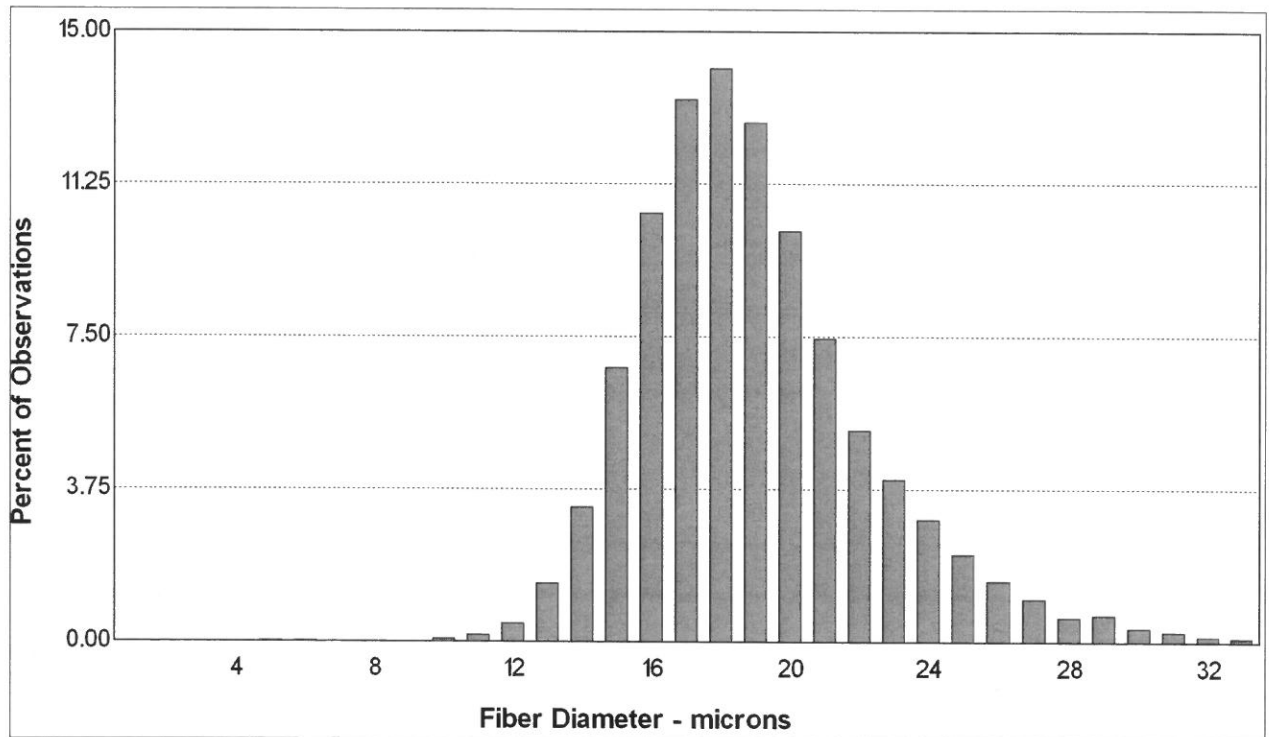

This Test Performed According to I.W.T.O Method 47