



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaka Zuchtverband Deutschland e.V./Claudia Böge
Buchholz 7
24306 Lebrade Germany

Date: 04/30/19


Test No: 974112

Animal and Sample Description

Animal Name: A17 WLA May Flower (276093480007425)	Animal ID: 9001700378
Breed: Alpaca(Huacaya)	Sample Location: L Flank
Sex: Female	Sample Date: 07/24/17
Color: White	Age: 05/19/17

Laboratory Data

Mean Fiber Diameter: 22.3 microns	Fibers Greater Than 30 microns: 3.9 %
Standard Deviation: 4.3 microns	Comfort Factor: 96.1 %
Coefficient of Variation: 19.3 %	Mean Curvature: 38.4 deg/mm
Spin Fineness: 21.4 microns	SD Curvature: 20.3 deg/mm

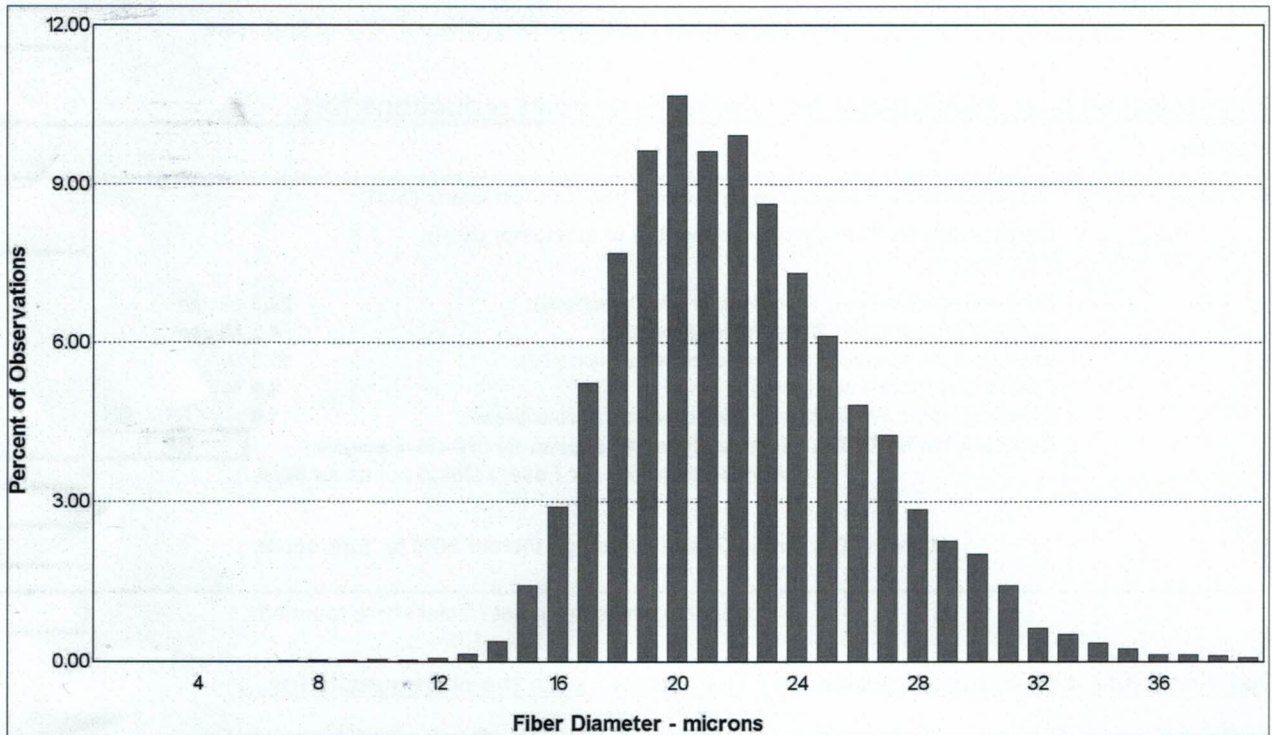

This Test Performed According to I.W.T.O Method 47

